



Designation: E2769 – 22

Standard Test Method for Elastic Modulus by Thermomechanical Analysis Using Three-Point Bending and Controlled Rate of Loading¹

This standard is issued under the fixed designation E2769; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method describes the use of linear controlled-rate-of-loading in three-point bending to determine the elastic modulus of isotropic specimens in the form of rectangular bars using a thermomechanical analyzer (TMA).

NOTE 1—This method is intended to provide results similar to those of Test Methods D790 or D5934 but is performed on a thermomechanical analyzer using smaller test specimens. Until the user demonstrates equivalence, the results of this method shall be considered independent and unrelated to those of Test Methods D790 or D5934.

1.2 This test method provides a means for determining the elastic modulus within the linear region of the stress-strain curves (see Fig. 1). This test is conducted under isothermal temperature conditions from -100°C to 300°C .

1.3 Typical test specimens are in the form of thin strips 0.5 mm in thickness, 1.5 mm in width, and 6 mm in length. The size of the test specimen is limited by the distance between the supports used in the three-point bending mode of operation, commonly 0.5 cm.

1.4 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

- D618 Practice for Conditioning Plastics for Testing
- D790 Test Methods for Flexural Properties of Unreinforced and Reinforced Plastics and Electrical Insulating Materials
- D5934 Test Method for Determination of Modulus of Elasticity for Rigid and Semi-Rigid Plastic Specimens by Controlled Rate of Loading Using Three-Point Bending (Withdrawn 2009)³
- E473 Terminology Relating to Thermal Analysis and Rheology
- E1142 Terminology Relating to Thermophysical Properties
- E1363 Test Method for Temperature Calibration of Thermomechanical Analyzers
- E2092 Test Method for Distortion Temperature in Three-Point Bending by Thermomechanical Analysis
- E2113 Test Method for Length Change Calibration of Thermomechanical Analyzers
- E2206 Test Method for Force Calibration of Thermomechanical Analyzers

3. Terminology

3.1 *Definitions*—Definitions of technical terms used in this standard are defined in Terminologies E473 and E1142 including anisotropic, Celsius, expansivity, isotropic, proportional limit, storage modulus, strain, stress, thermodilatometry, thermomechanical analysis, and yield point.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *elastic modulus, n* —the ratio of stress to corresponding strain within the elastic limit on the stress-strain curve (see Fig. 1) expressed in Pascal units.

4. Summary of Test Method

4.1 A specimen of rectangular cross section is tested in three-point bending (flexure) as a beam. The beam rests on two

¹ This test method is under the jurisdiction of ASTM Committee E37 on Thermal Measurements and is the direct responsibility of Subcommittee E37.10 on Fundamental, Statistical and Mechanical Properties.

Current edition approved Feb. 1, 2022. Published September 2022. Originally approved in 2011. Last previous version approved in 2018 as E2769 – 18. DOI: 10.1520/E2769-22.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

*A Summary of Changes section appears at the end of this standard

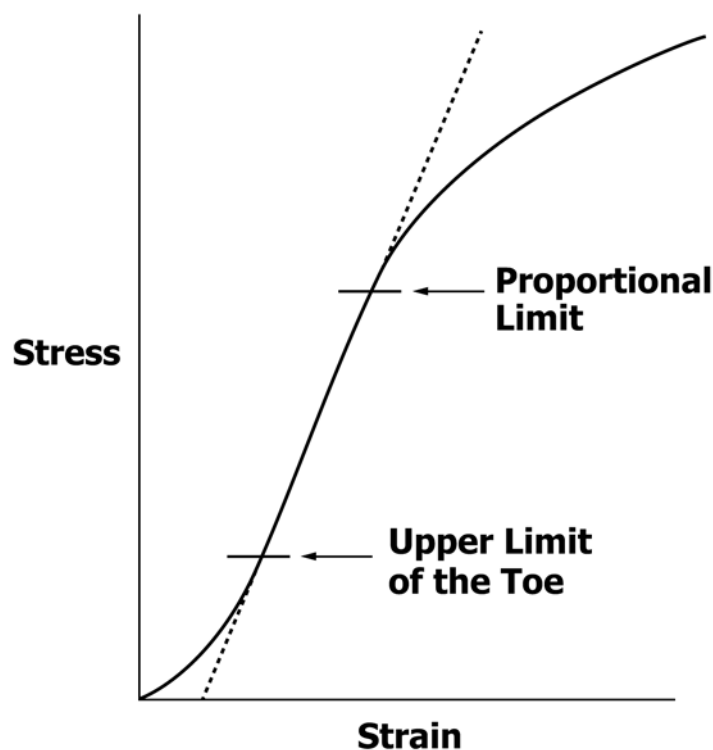


FIG. 1 Stress-Strain Curve (Linear Region)

supports and is loaded midway between the supports by means of a loading nose. A linearly increasing load (stress) is applied to the test specimen of known geometry while the resulting deflection (strain) is measured under isothermal conditions. The elastic modulus is obtained from the linear portion of the display of resultant strain versus applied stress.

5. Significance and Use

5.1 This test method provides a means of characterizing the mechanical behavior of materials using very small amounts of material including thermoplastic and thermoset polymers, composites, and metals.

5.2 The data obtained may be used for research and development and establishment of optimum processing conditions. The data are not intended for use in design or for predicting performance.

NOTE 2—This test method may not be suitable for anisotropic materials.

6. Interferences

6.1 Since small test specimen geometries are used, it is essential that the specimens be representative of the material being tested.

6.2 This test method is not applicable for strains greater than 3 %.

7. Apparatus

7.1 The function of the apparatus is to hold a rectangular test specimen (beam) so that the material acts as the elastic and dissipative element in a mechanically driven linear displacement system. Displacements (deflections) are generated using a

controlled loading rate applied to a specimen in a three-point bending configuration.

7.2 *Thermomechanical Analyzer*—The essential instrumentation required to provide the minimum thermomechanical analytical or thermomechanometric capability for this method includes:

7.2.1 A rigid *specimen holder* of inert low expansivity material $\leq 30 \mu\text{m m}^{-1} \text{K}^{-1}$ to center the specimen in the furnace and to fix the specimen to mechanical ground.

7.2.2 A rigid *flexure fixture* of inert low expansivity material $\leq 30 \mu\text{m m}^{-1} \text{K}^{-1}$ to support the test specimen in a three-point bending mode (see Fig. 2). The radius of the supports shall not be greater than 1 mm.

7.2.3 A rigid *knife-edge compression probe* of inert low expansivity material $\leq 30 \mu\text{m m}^{-1} \text{K}^{-1}$ that contacts the specimen with an applied compressive force (see Fig. 1). The radius of the knife-edge shall not be larger than 1 mm.

7.2.4 *Deflection sensing element*, having a linear output over a minimum range of 5 mm to measure the displacement of the rigid compression probe (see 7.2.3) to within $\pm 0.1 \mu\text{m}$.

7.2.5 *Programmable weight or force transducer* to generate a force program of 0.1 N min^{-1} over the range of 0.01 to 1.0 N that is applied to the specimen through the rigid compression probe (see 7.2.3).

7.2.6 *Temperature sensor*, that can be reproducibly positioned in close proximity to the specimen to measure its temperature with the range between -100°C and 300°C to within $\pm 0.1^\circ\text{C}$.

NOTE 3—Other temperatures may be used but shall be reported.